

S.I.N. Components are intended for expert procedures, which must be performed by qualified professionals. The use of the product and surgical techniques are inherent to the professional's training. The use of the product must be performed in a surgical environment and in proper conditions for the health and safety of the patient.



PRODUCT DESCRIPTION

Healing Cap: It consists of a cylindrical abutment, its lower end adapts to the implant connection and has a thread for fixation. They are manufactured in titanium grade V and sold in sterile form.

Protector: It consists of a cylindrical abutment, its lower end adapts to the abutment (prosthetic intermediary) and has a thread for fixation. They are manufactured in titanium grade V and sold in sterile form.

Implant Cover Screw: It consists of a cylindrical titanium grade V abutment available for external hexagon, internal hexagon and cone morse and has a thread for fixing the implant.

The chemical composition of the Dental Components is according to ASTM F136:

Chemical Element	Composition % (mass/mass)
Nitrogen	≤ 0.05
Carbon	≤ 0.08
Hydrogen	≤ 0.012
Iron	≤ 0.25
Oxygen	≤ 0.13
Aluminum	5.5 - 6.5
Vanadium	3.5 - 4.5
Titanium	Balance

INDICATIONS OF USE

Healing Cap: Indicated to guide proper healing of the perimplant gum tissue, conditioning the space of the dental prosthesis in the patient's gums. It is also intended to leave the implant platform free for the next procedures.

Protector: Recommended to guide the appropriate healing of the perimplant gingival tissue, conditioning the space of the dental prosthesis in the patient's gingiva.

Implant Cover Screw: Its use is indicated to protect the interior of the implant until the installation of the prosthesis, against any contaminant particle that may enter its orifice.

The S.I.N. Components are indicated to be used up to 30 days.

PURPOSE AND OPERATION PRINCIPLE

Healing Cap / Protector: Its purpose is to form the emergence profile for correct seating of the prosthesis, besides protecting the interior of the implant from intra-oral contamination. They are based on the principle of stabilization and epithelialization of the gum tissue.

Implant Cover Screw: Its purpose is to protect the interior of the implant from intra-oral contamination.

HOW TO USE THE COMPONENT

After implant installation or after reopening procedure:

- Carefully evaluate the fibromucosal tissue, its thickness and muco-gingival biotype, to select the height of the component to be used;
- Radiograph for precision in locating the implant with an appropriate radiographic technique (parallelism or bisector - periapical X-ray);
- Check the implant diameter;
- Check the angulation of the installed implant;
- Calculate the height of the healers, using a millimeter probe according to the height of the fibromucosa in its crest up to the implant platform, and the healer must be approximately 2mm higher than this measurement;
- Remove the component from the packaging and adapt it to the implant platform with the help of digital wrenches, counter-angle wrenches or ratchet wrenches. Screw the implant in until it is fully seated with a digital torque of 10N.cm.
- Note that the diameter of the components varies according to the rehabilitated region, tooth to be replaced, prosthetic space, implant diameter, ridge thickness, and if there is more than one implant, the space between them, in order to preserve the interproximal tissue for papilla formation;
- The healers must be left in the oral cavity for approximately 15 days;



ATTENTION

The S.I.N. Components are intended for expert procedures, which must be performed by qualified professionals in implant Dentistry. The product must be used in a surgical environment and in proper conditions for the health and safety of the patient.

PRECAUTIONS

Consider the general health of the patient, the same must undergo a thorough clinical analysis. Failure to perform the pre-surgical evaluation can lead to the impossibility of finding pre-existing diseases. Patients with local or systemic factors that may interfere with the soft tissue healing process should receive special attention. Sterilization of the S.I.N. Components is only guaranteed if the primary packaging (blister) is not damaged. Do not use the product if the packaging has been tampered with. Only open the package at the time of surgery and use the product immediately. Handle the material only in a sterile field. All material used in the procedure must be sterile. Components not used after opening the carton should be discarded. Products

with expired validity should not be used. During the surgical and prosthetic procedure only use implants, components and instruments specified by S.I.N., they have specific dimensions and tolerances for each implant system guaranteeing longevity of the product. Other brandcomponents or adapted to the implant models can reduce the life of the system causing irreversible damage. The platform of the S.I.N. Components that adapts to the implant must not be altered in any way. The professional must ensure the patient does not aspirate the product. It is the responsibility of the professional to use S.I.N. in accordance with the instructions for use, as well as to determine if it is appropriate to the individual situation of each patient. If a correct diameter is not used, soft tissue irritation may occur. The patient should be informed about all possible surgical complications, contraindications, warnings, precautions and adverse reactions. All documentation accompanying the product should also be made available to the customer. The professional must inform the patient about the correct form of cleaning, the need for regular monitoring, avoiding physical and mechanical tensions and not subjecting the product to inappropriate efforts.

RECOMMENDATIONS

For the placement of S.I.N. Components, it is recommended that the professional have a specialization course in the area and prepare a prosthetic execution plan. Inadequate planning and/or lack of occlusal adjustment may compromise the performance of the implant/prosthesis combination resulting in system failure, such as implant loss or fracture, loosening or fracture of the prosthetic screws. The diameter and the angulation of the implant, as well as the gingival height, must be taken into account when choosing the model of S.I.N. Components to be used. The S.I.N. does not recommend implant installation in patients with inadequate oral hygiene, uncooperative and unmotivated patients, drug or alcohol abuse, psychoses, chemical dependence, prolonged functional disorders that resist any drug treatment, xerostomia, low immune system, diseases which require the use of steroids regularly, endocrinological diseases, drug allergy, diabetes mellitus, anticoagulants/bleeding diathesis, bruxism, other parafunctional habits, tobacco abuse, installation in children and pregnant women and during breastfeeding.

CONTRAINdications

The use of S.I.N. Components is contraindicated in cases of chronic periodontal inflammation, a patient not prepared to undergo oral rehabilitation, inappropriate parafunctional habits, for example bruxism, untreatable occlusion/joint problems, active intraoral infection and in the case of immediate loading, primary implant stability inadequate.

SIDE EFFECTS

The installation recommendations must be followed for the proper functioning of the product, if not, the final result can be compromised generating, loss or fracture of the part. The product can cause transient side effects due to compression of perimplant tissues such as, slight bleeding, edema, pain, discomfort or even infection in case of breaking aseptic barrier.

WARNING

The implants must receive components with compatible geometry or specific components for the technique switching platform and installation indication compatible only with S.I.N. system. The

products are for single use and cannot be re-sterilized and/or reused. The reuse or re sterilization of this product may cause contagious infectious disease, deformation and wear of the product.

TRACEABILITY

All S.I.N. products have sequential lots that allow traceability, which promotes greater safety for the professional qualified to the procedure. Through this batch number, it is possible to know the entire history of the product from the manufacturing process to the distribution time. The components are available with three (3) way traceability labels.

STORAGE

The S.I.N. medical device should be stored in a cool dry place at a temperature of 15°C to 35°C and protected from direct sunlight in their original unopened packaging and should not be damaged.

HANDLING

The S.I.N. Components are sterile products that should be handled only in a sterile field by properly trained professionals and in appropriate scrubs at the time of the surgical procedure.

DISPOSAL OF MATERIAL

The disposal of materials should comply with local hospital regulations and applicable local laws.

TRANSPORTATION

The S.I.N. Components must be transported adequately to avoid falling and stored under a maximum temperature of 35°C, protected from heat and moisture. Carriage must be carried out in its original packaging.

COMPLEMENTARY INFORMATIONS

Magnetic Resonance Imaging (MRI): Non-clinical testing and in vitro electromagnetic simulations demonstrated that the S.I.N. devices are MR Conditional.

CAUTION: Patient imaging can only be obtained by delimiting at least 30cm from the implant or ensuring that the implant is located outside the radiofrequency coil.

A patient with this device can be safely scanned on an MRI system under the following conditions:

Device Name	S.I.N. Implant System
Static Magnetic Field Strength (B0)	≤ 3.0 T
Maximum Spatial Field Gradient	50 T/m (5.00 gauss/cm).
RF Excitation	Circularly Polarized (CP)

RF Transmit Coil Type	Head coil and body coil permitted. Extremity T/R coils permitted.
Operating Mode	Normal Operating Mode in the allowed imaging zone
Maximum Whole-Body SAR	2.4 W/kg (15 minutes of scanning, Normal Operating Mode)
Maximum Head SAR	2.0 W/kg (15 minutes of scanning, Normal Operating Mode)
Scan Duration	15 minutes
Temperature Rise	Maximum temperature rise of 0.45 °C/(W/kg), after 15 minutes of continuous scanning in a static magnetic field of 3 T with either head type or body type coils
Artifact	When imaged using a gradient-echo sequence and a 3 T MR system, image artifact can extend up to approximately 12 mm with a body coil type, and up to approximately 32 mm with a head coil type


Product Exclusively for Odontological use. Reprocessing not allowed. Any serious incident that has occurred in relation to the device should be reported to the manufacturer and competent authority of the country in which the dentist and/or patient is established. If you need the printed version of this instruction for use, without any cost, please request by e-mail to sin@sinimplantsystem.com or call to 0800 770 8290 will receive until 7 days calendar.

TRACEABILITY LABELS

The S.I.N. Components are available from S.I.N. with 3 (three) labels containing product information. The labels must be used as follows:

Tax Documentation Label: The dental surgeon must stick a label on the implant's tax documentation.

Medical Record Label: The dental surgeon must paste a label in the patient's medical record in order to maintain traceability of the products used.

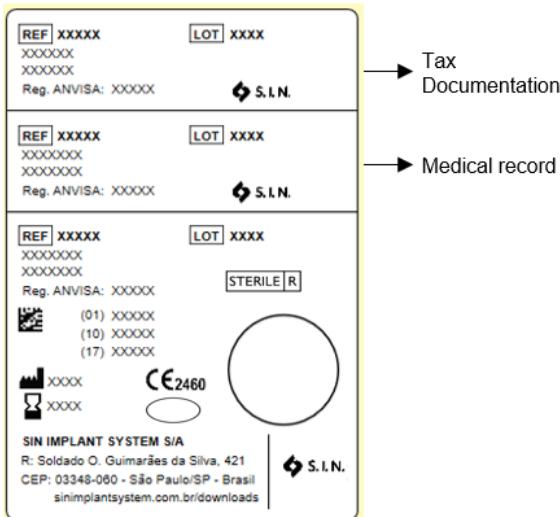

*Merorially illustrative image

STERILE R

FORM OF PRESENTATION AND STERILIZATION

This product is supplied sterile and single-use (sterilization method: gamma radiation) packaged in a unit that offers double protection: secondary packaging (cardboard) and primary blister packaging (PET film and surgical grade paper).

EXPIRATION DATE

The information regarding the expiration date can be found on the labeling of the product. After installation on the patient, the product must be monitored by the professional.

STERILE	PRODUTO ESTERILIZADO POR RADIAÇÃO GAMA	PRODUCT STERILIZED THROUGH GAMMA RAYS	PRODUCTO ESTERILIZADO POR RADIACIÓN GAMA
	NÃO REUTILIZAR	DO NOT REUSE	NO LO REUTILICE
	CONSULTAR AS INSTRUÇÕES DE USO	CONSULT INSTRUCTIONS FOR USE	CONSULTE LAS INSTRUCCIONES DE USO
	MARCAÇÃO CE	CE MARK	MARCA CE
	MANTENHA SECO	KEEP DRY	MANTÉNGALO SECO
	MANTENHA AO ABRIGO DO SOL	KEEP AWAY FROM SUNLIGHT	MANTÉNGALO LEJOS DE LA LUZ SOLAR
	NÃO UTILIZAR SE A EMBALAGEM ESTIVER VIOLADA	DO NOT USE IF PACKAGE IS DAMAGED	NO LO UTILICE SI EL ENVOLTORIO ESTÁ DAÑADO
	NÃO REESTERILIZE	DO NOT RESTERILIZE	NO LO REESTERILIZAR
	ATENÇÃO	CAUTION	PRECAUCIÓN
EU REP	REPRESENTANTE AUTORIZADO NA COMUNIDADE EUROPEIA	AUTHORIZED REPRESENTATIVE IN THE EUROPEAN COMMUNITY	REPRESENTANTE AUTORIZADO EN LA COMUNIDAD EUROPEA
	LIMITE DE TEMPERATURA	TEMPERATURE LIMIT	LÍMITE DE TEMPERATURA
Rx only	ATENÇÃO: A LEI FEDERAL (EUA) LIMITA A VENDA DESTE DISPOSITIVO POR OU POR ORDEM DE UM PROFISSIONAL DE SAÚDE LICENCIADO.	CAUTION: FEDERAL LAW (USA) RESTRICTS THIS DEVICE TO SALE BY OR ON THE ORDER OF A LICENSED HEALTHCARE PRACTITIONER.	PRECAUCIÓN: LAS LEYES FEDERALES (USA) RESTRINGEN LA VENTA DE ESTE DISPOSITIVO POR O EN EL ORDEN DE UN PROFESIONAL DE LA SALUD LICENCIADO.
	FABRICANTE	MANUFACTURER	FABRICANTE
	DATA DE FABRICAÇÃO	DATE OF MANUFACTURE	FECHA DE FABRICACIÓN
	VALIDADE	USE-BY DATE	VALIDEZ
REF	CÓDIGO DE REFERÊNCIA	REFERENCE CODE	CÓDIGO DE REFERÊNCIA
MD	DISPOSITIVO MÉDICO	MEDICAL DEVICE	DISPOSITIVO MEDICO
UDI	IDENTIFICADOR ÚNICO DO DISPOSITIVO	UNIQUE DEVICE IDENTIFIER	IDENTIFICADOR DE DISPOSITIVO ÚNICO
	SISTEMA DE BARREIRA ESTÉRIL	SINGLE STERILE BARRIER SYSTEM	SISTEMA DE BARRERA ESTÉRIL SIMPLES
	IMPORTADOR	IMPORTER	IMPORTADOR
	DISTRIBUIDOR	DESTRIIBUTOR	DISTRIBUIDOR

 BRA	PAÍS DE FABRICAÇÃO	COUNTRY OF MANUFACTURE	PAÍS DE FABRICACIÓN
 LOT	LOTE	BATCH CODE	LOTE
 RECYCLABLE	EMBALAGEM RECICLÁVEL	RECYCABLE PACKAGING	EMBALAJE RECICABLE
 MR CONDICIONAL	MR CONDICIONAL	MR CONDITIONAL	MR CONDICIONAL

**MANUFACTURER****S.I.N. Implant System LTDA**

CNPJ [Corporate Taxpayer's Registry]: 04.298.106/0001-74

Rua Soldado Ocimar Guimarães da Silva, 421 - Vila Rio Branco

CEP: 03348-060 - São Paulo - SP - Brasil

EU	REP
----	-----

OBELIS S.A.

Bd. Général Wahis 53

1030 Brussels, Belgium

**SERVICE TO PROFESSIONALS**

0800 770 8290 +55 (11) 2169-3000

www.sinimplantsystem.come-mail: sin@sinimplantsystem.com**RESPONSIBLE TECHNICIAN**

Alessio Di Risio

CREA-SP: 5061207169

PRODUCT

S.I.N. Components